

FIG. 1A

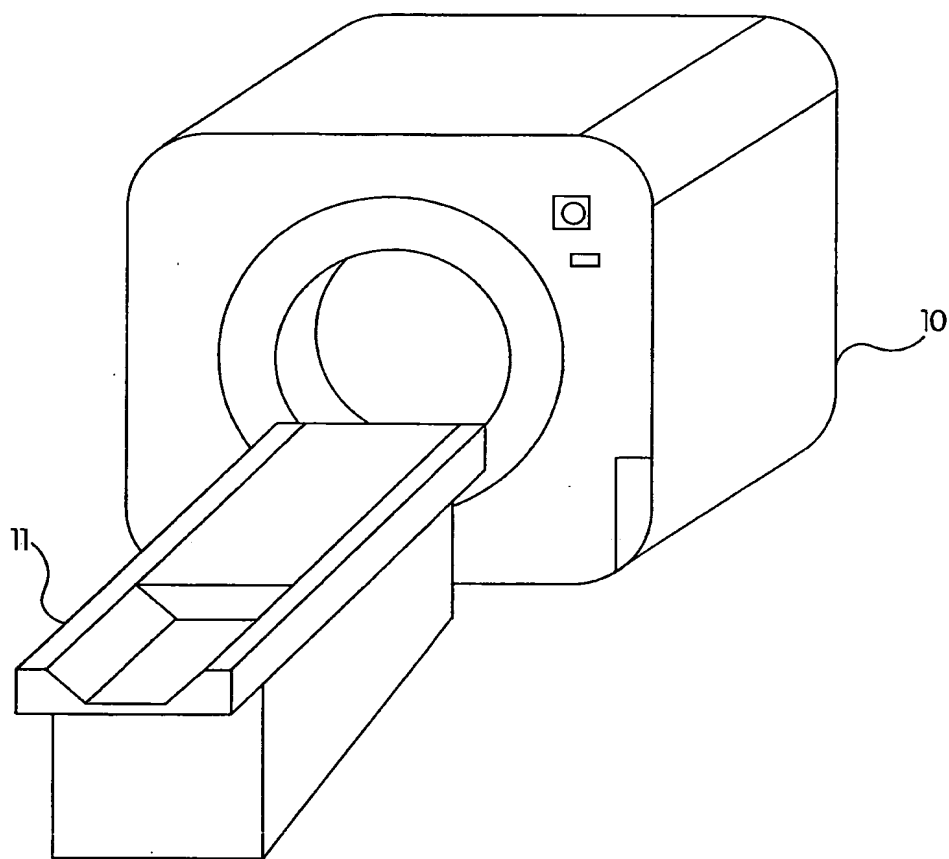


FIG. 1B

3/25

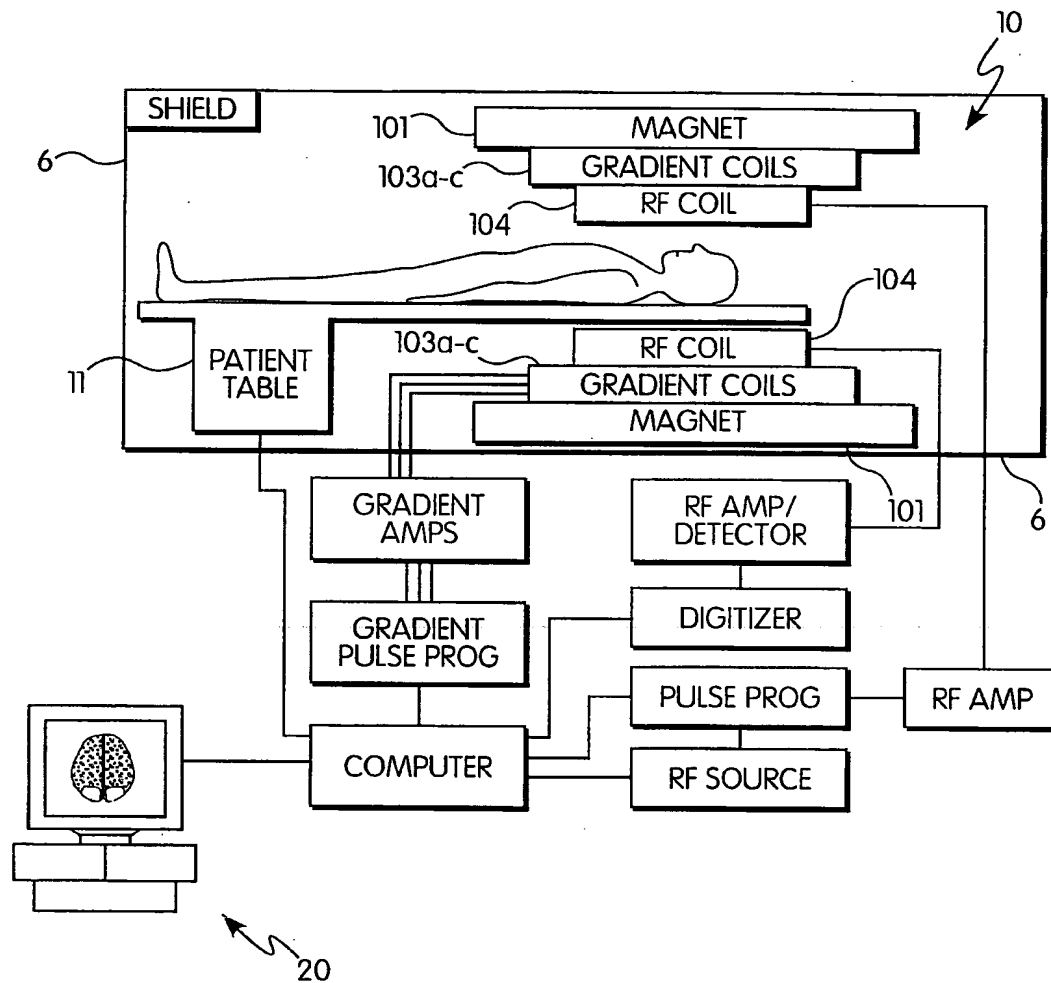


FIG. 1C

4/25





FIG. 2B

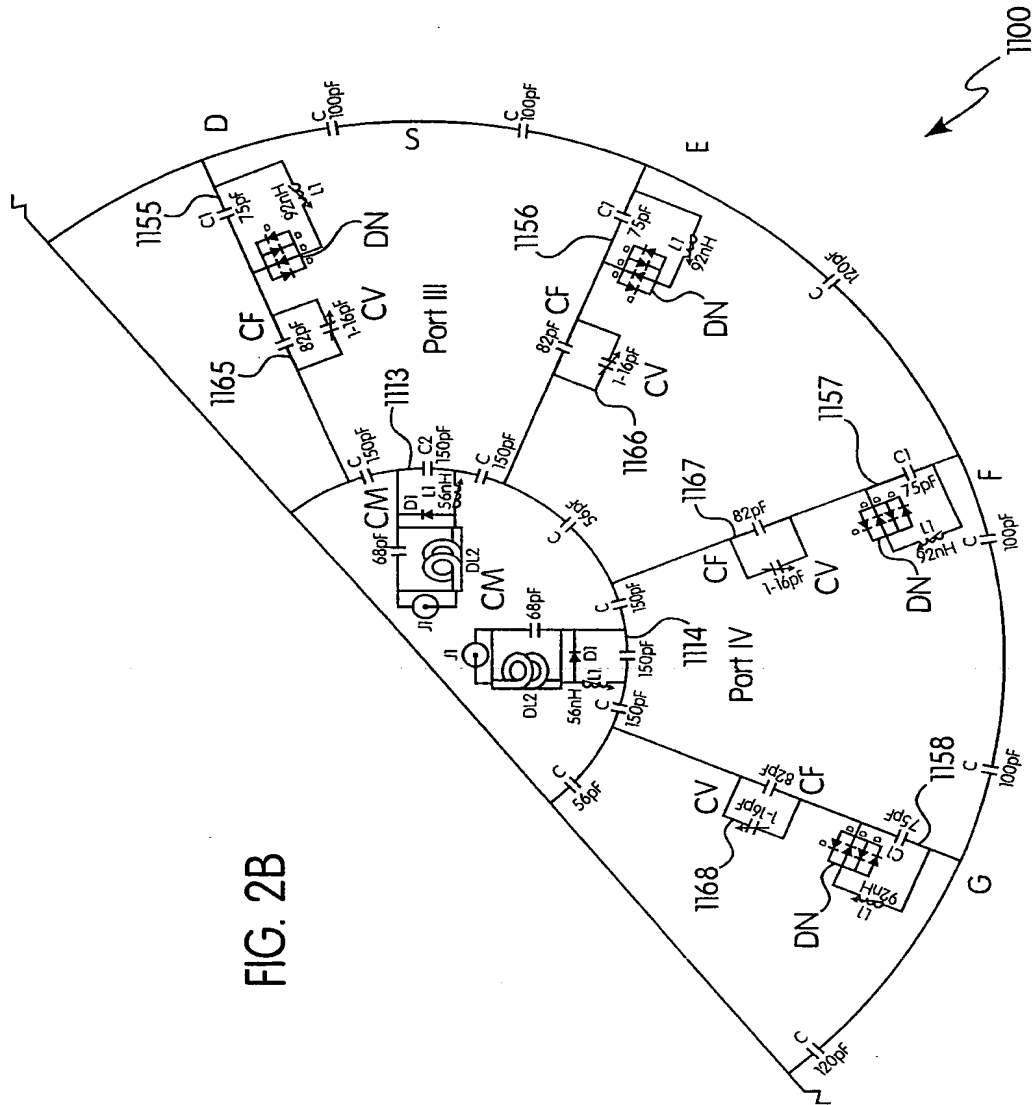

6/25

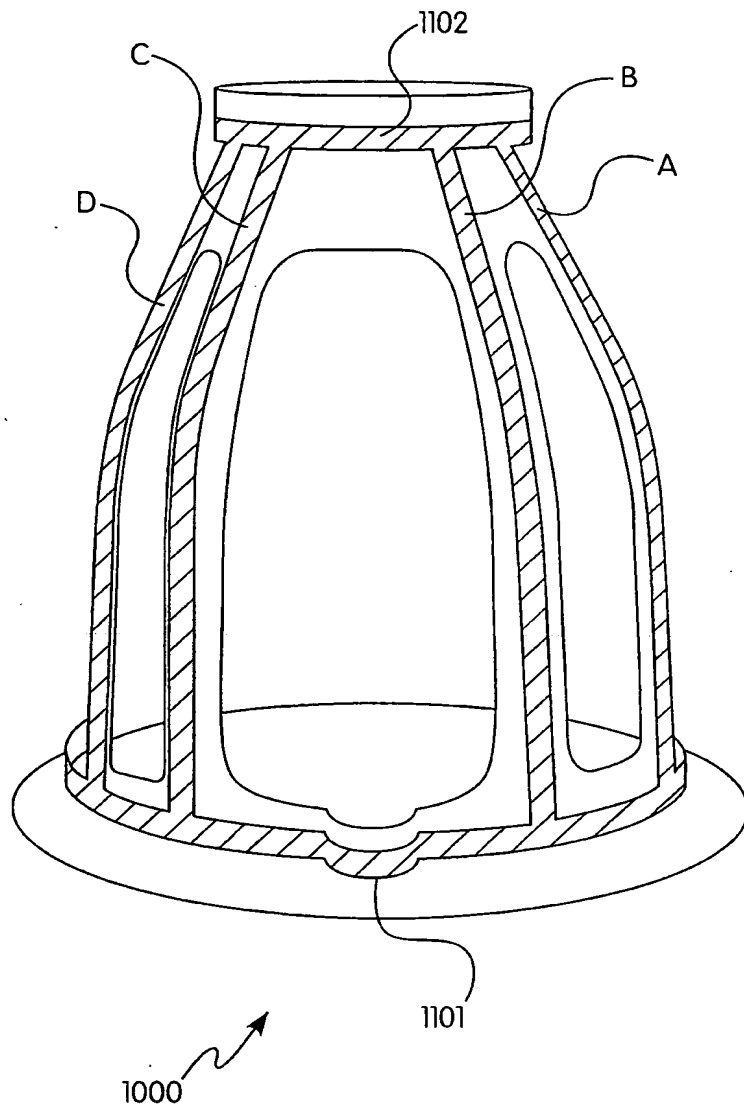


FIG. 3

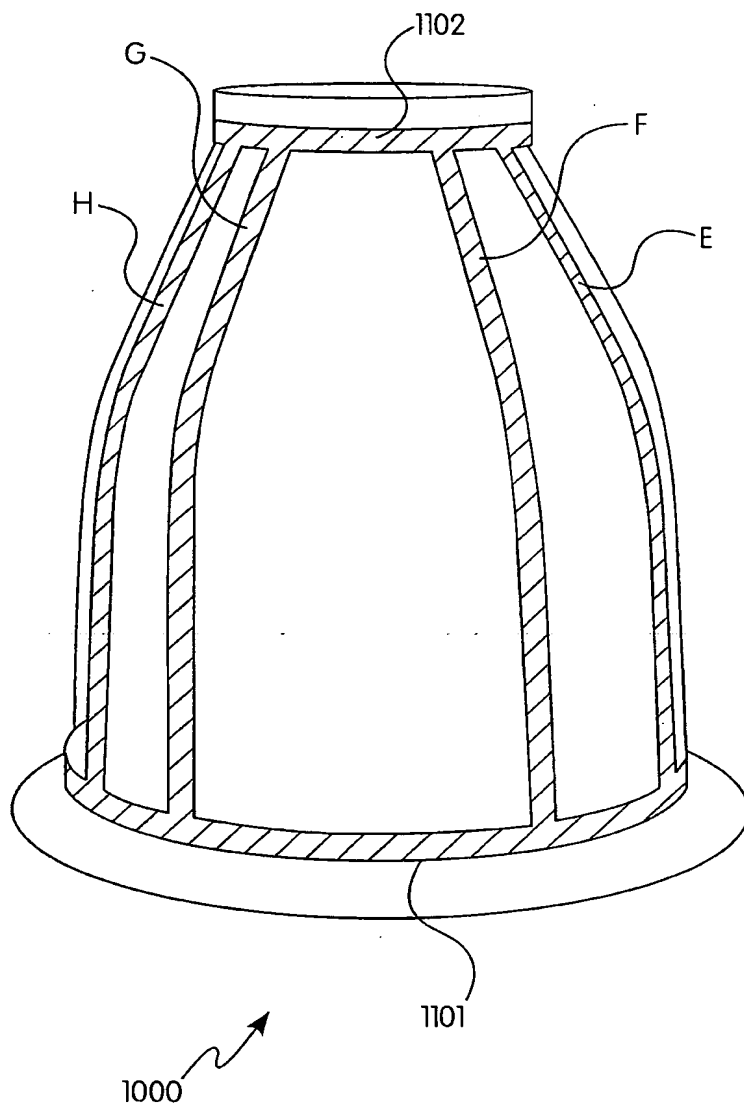


FIG. 4

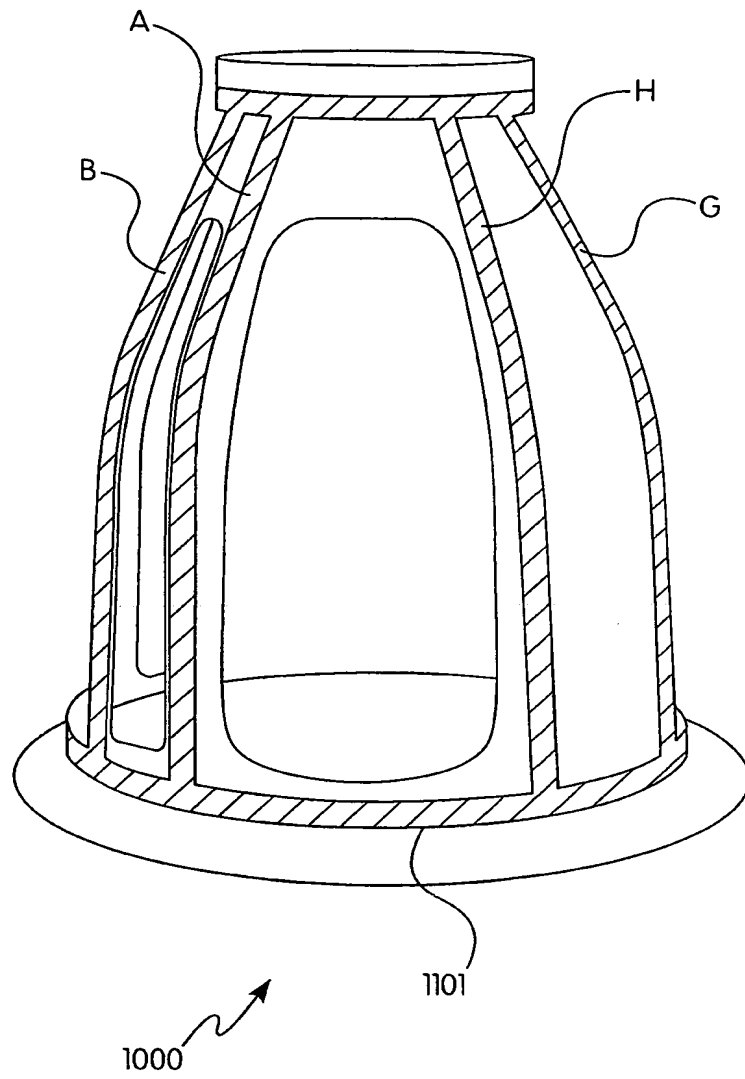


FIG. 5

9/25

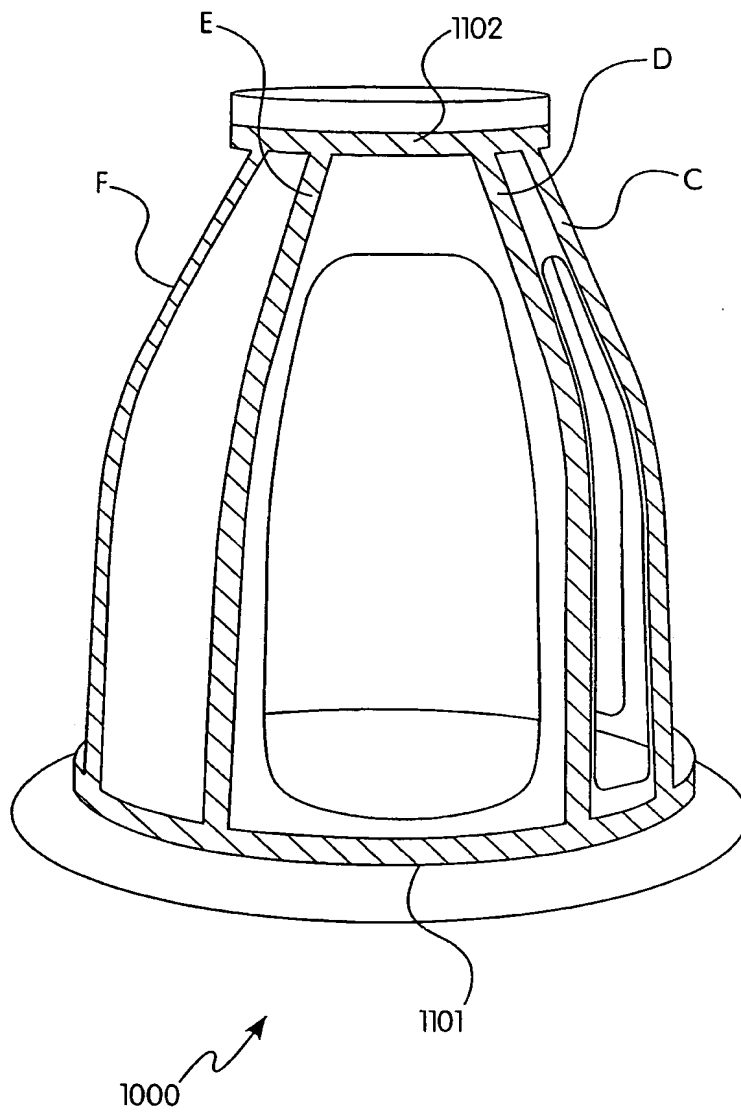


FIG. 6

10/25

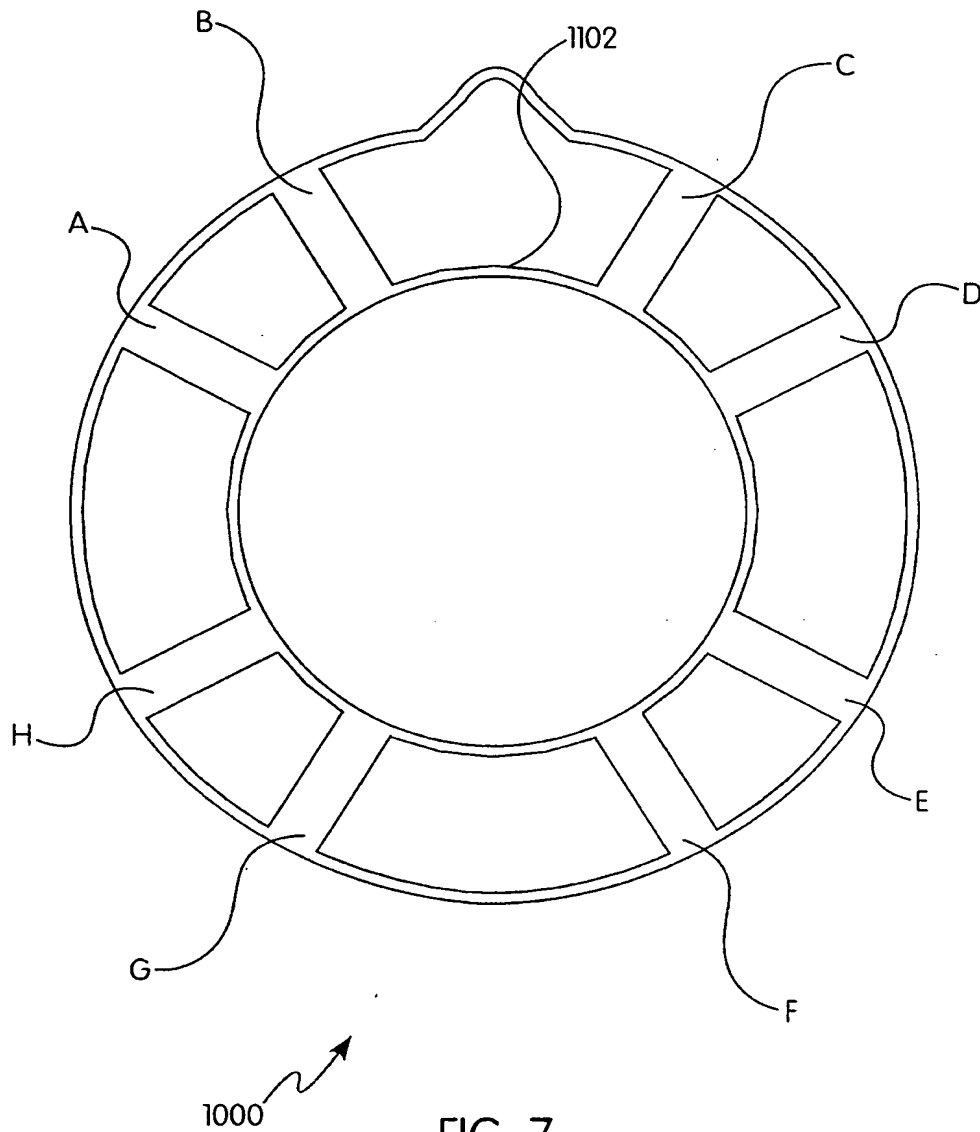


FIG. 7

11/25


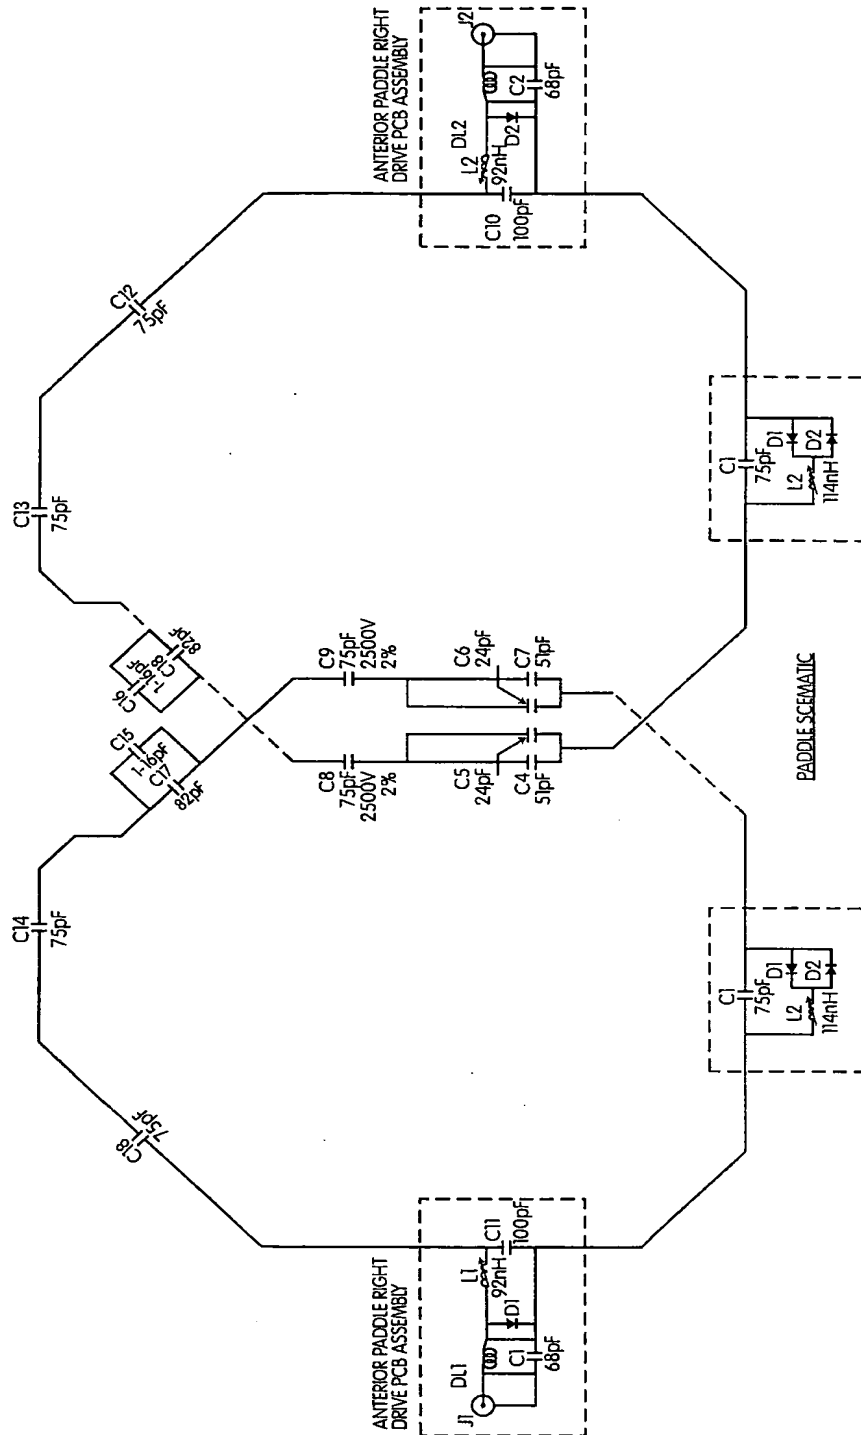



FIG. 8

12/25

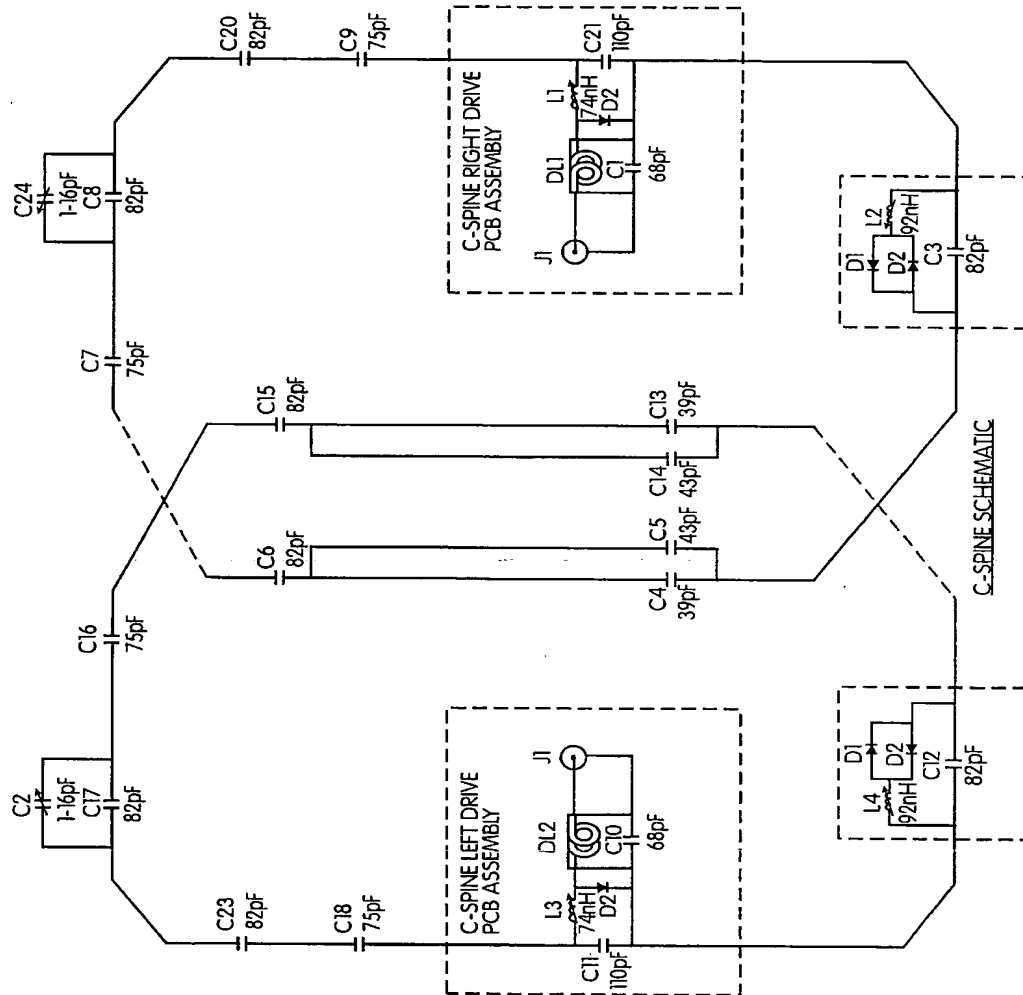

C-SPINE SCHEMATIC

FIG. 9

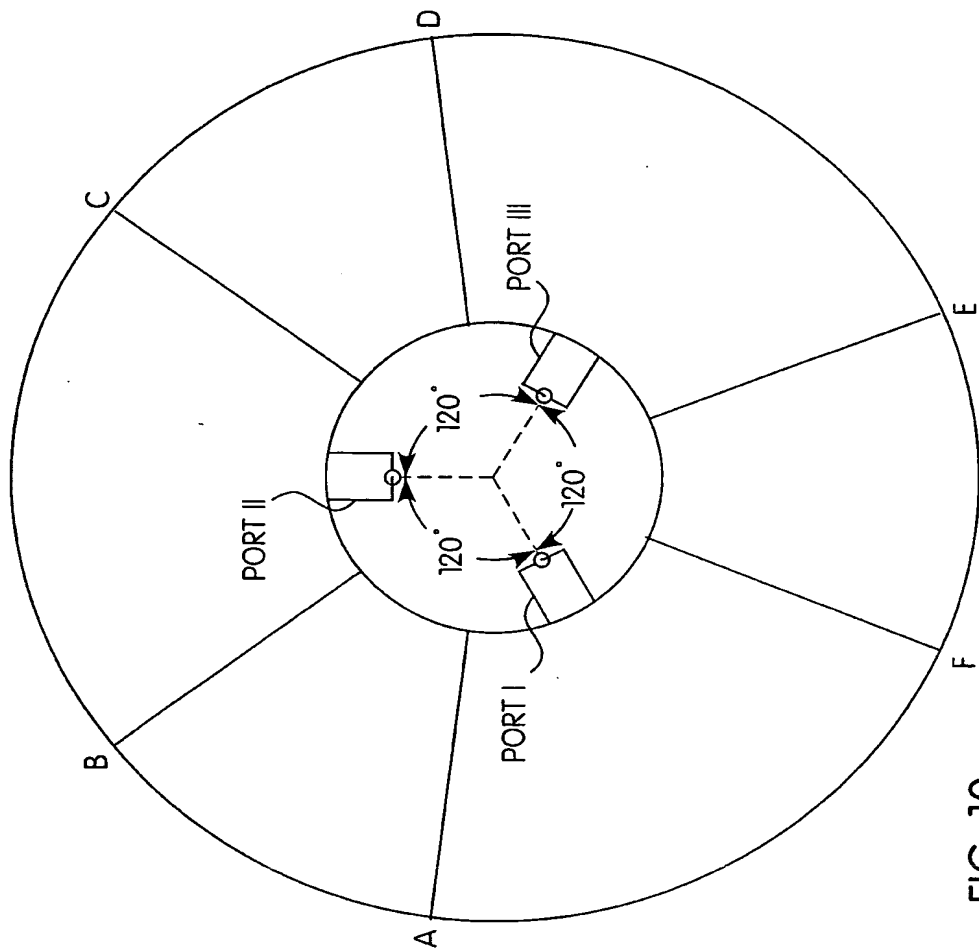

14/25

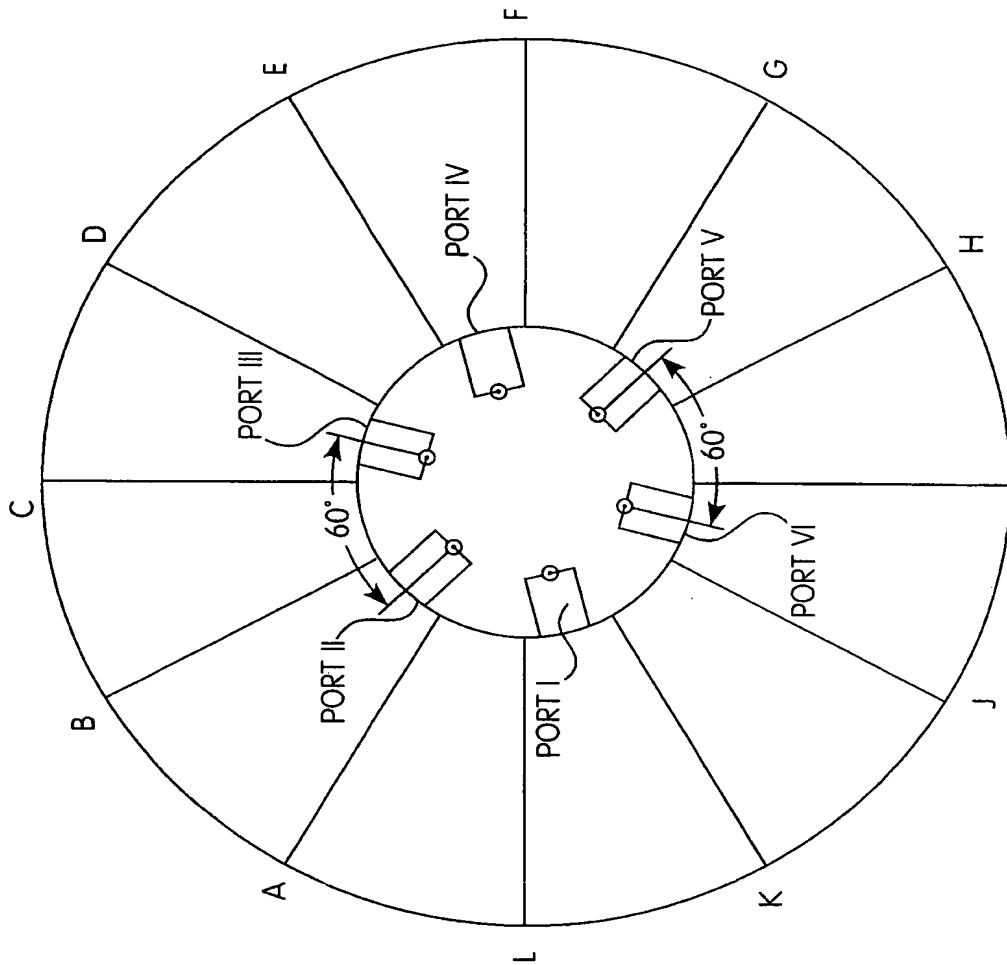


FIG. 11

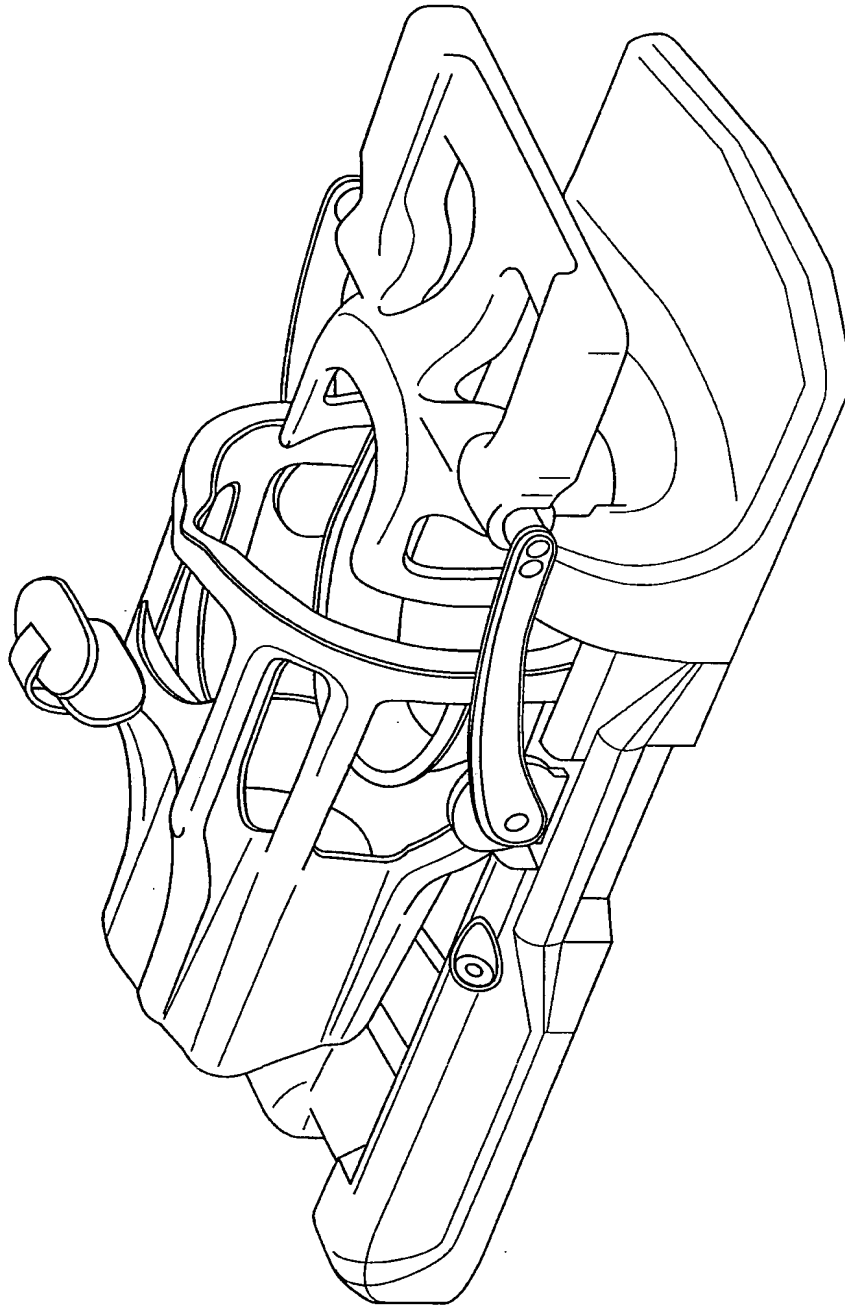


FIG. 12

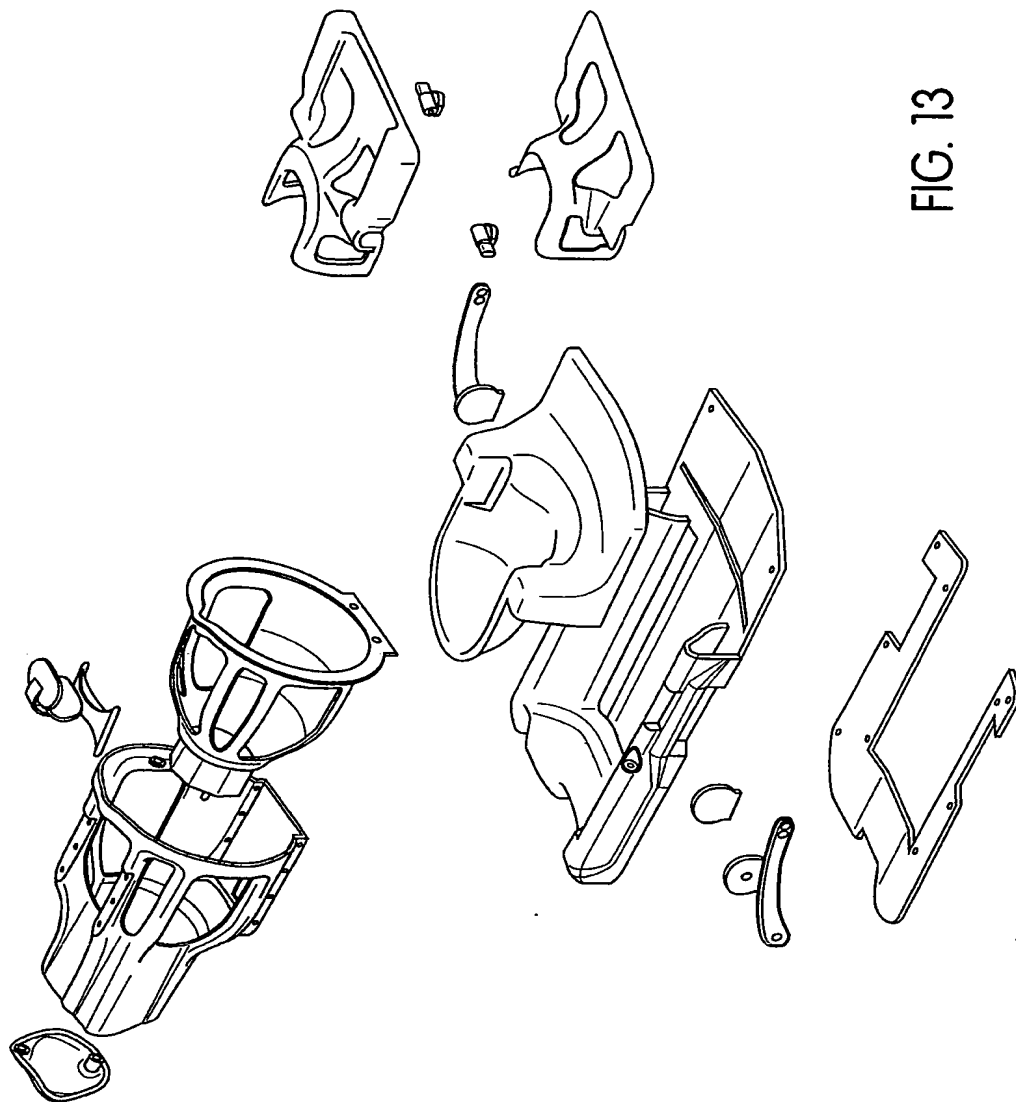


FIG. 13

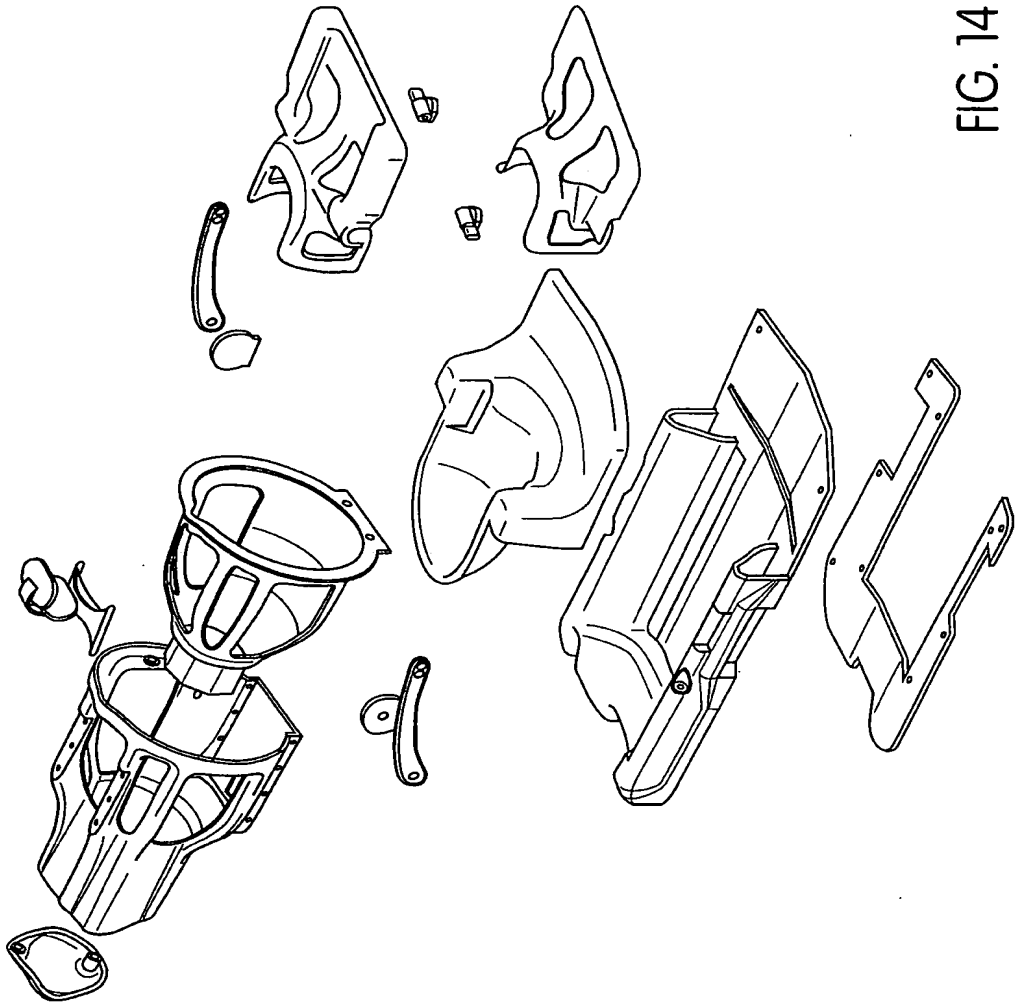


FIG. 14

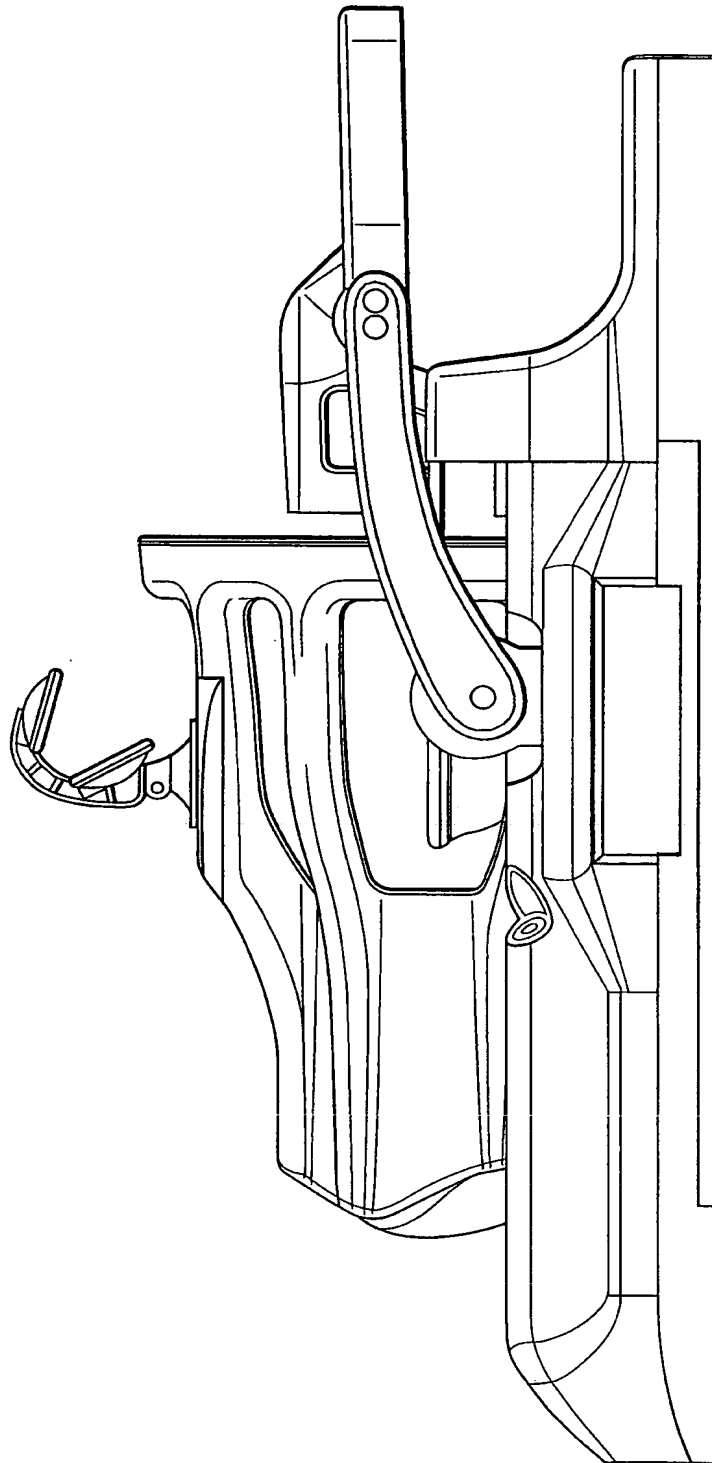


FIG. 15

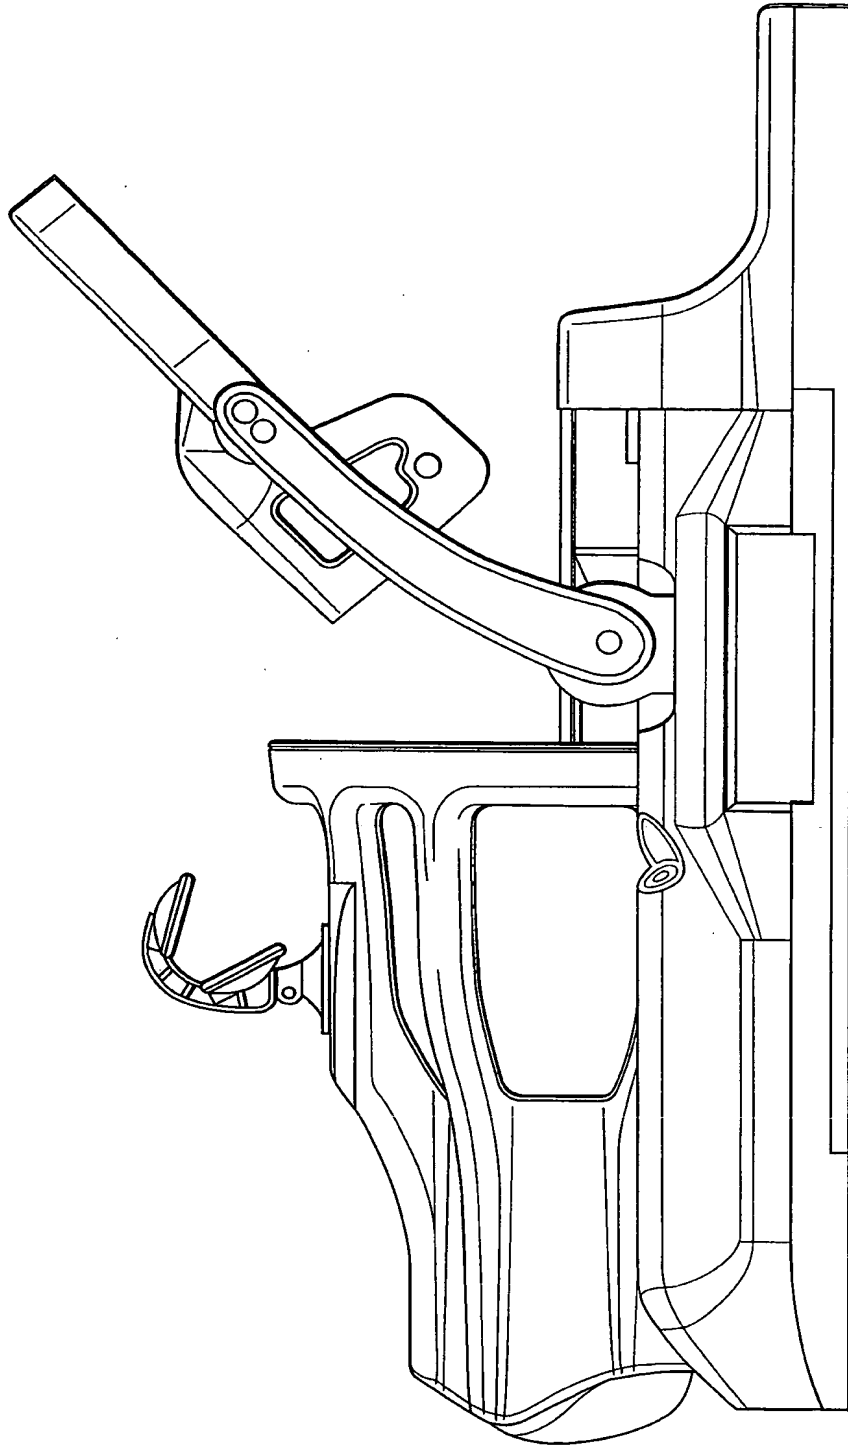


FIG. 16

20/25

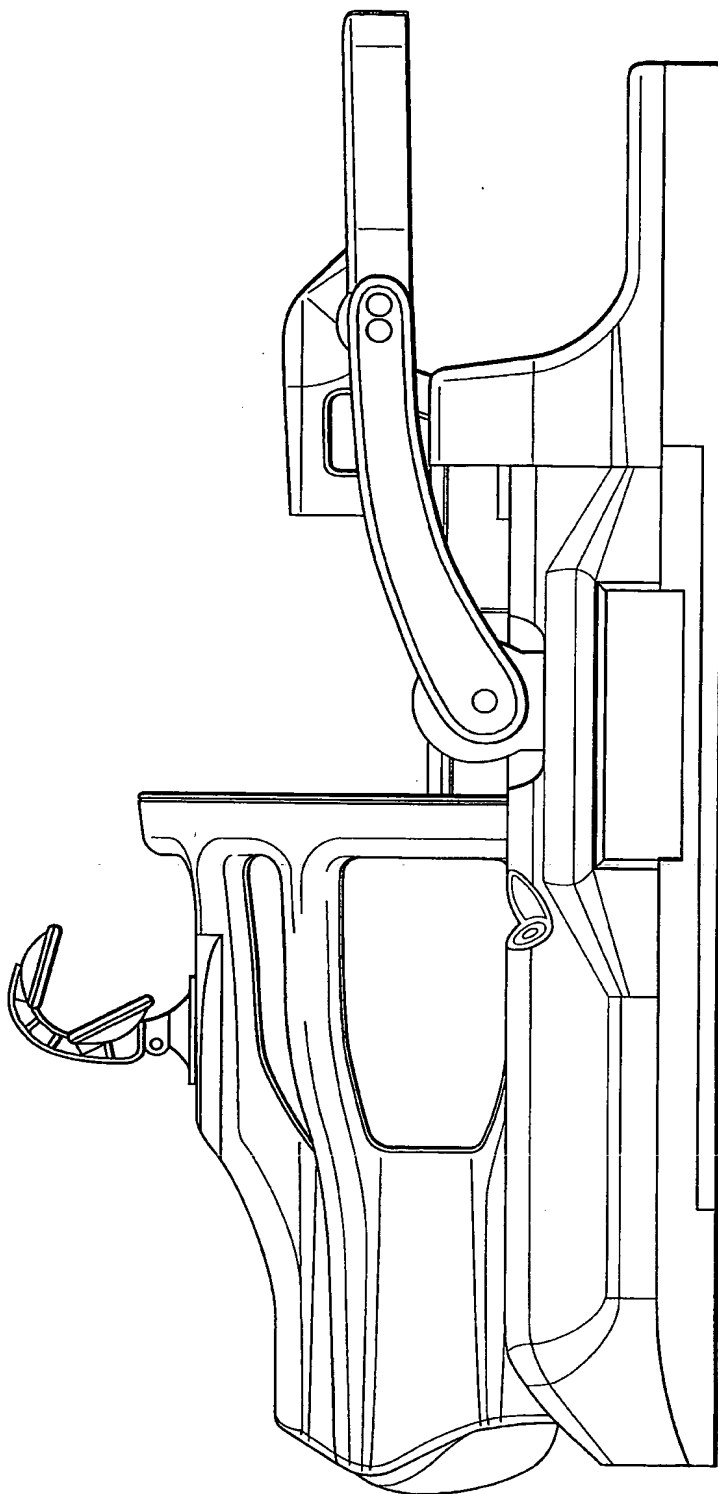


FIG. 17

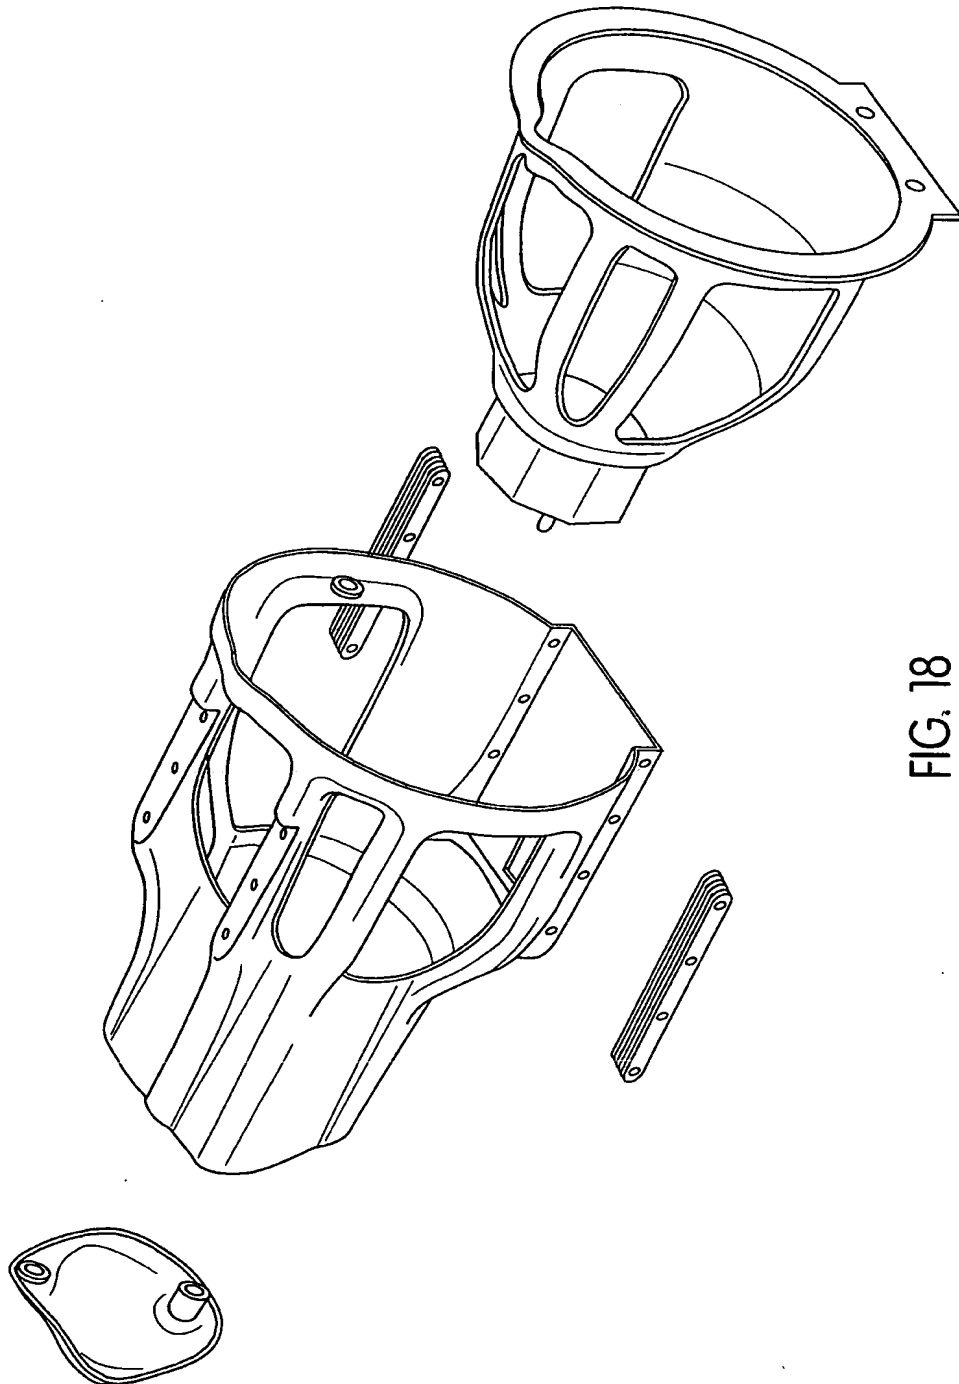


FIG. 18

PARALLEL IMAGING COMPATIBLE
BIRDCAGE RESONATOR
10/723,428
MR/02-003

22/25

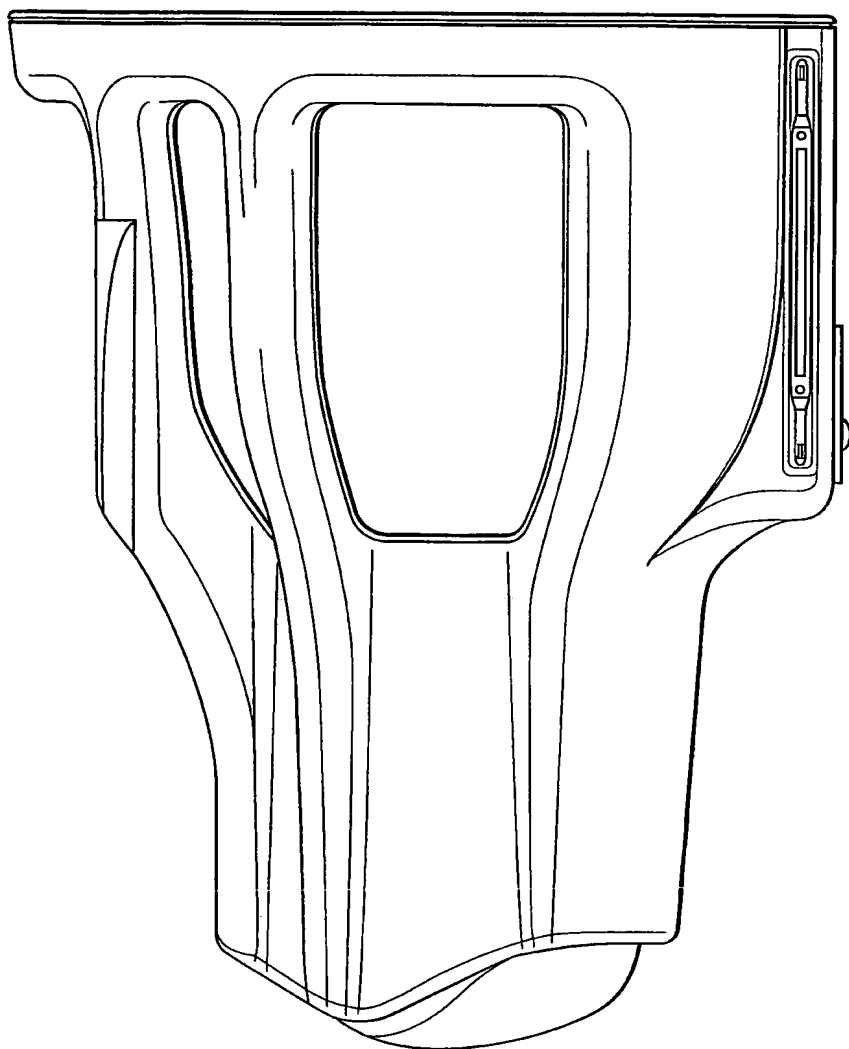


FIG. 19

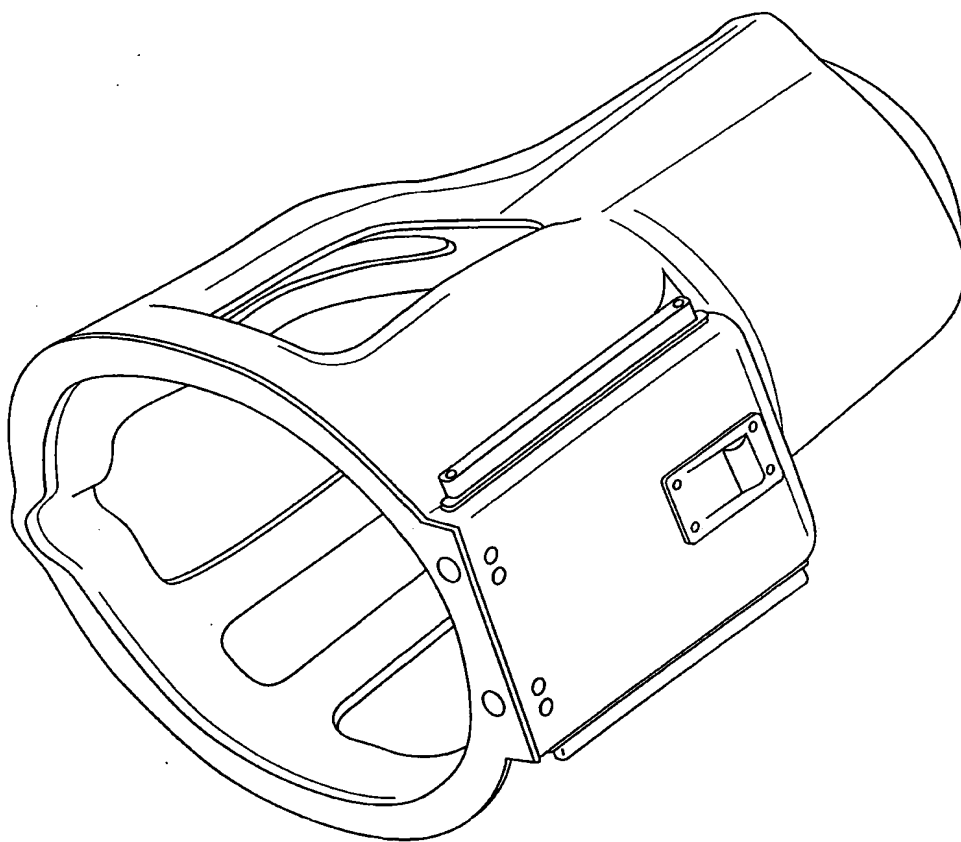


FIG. 20

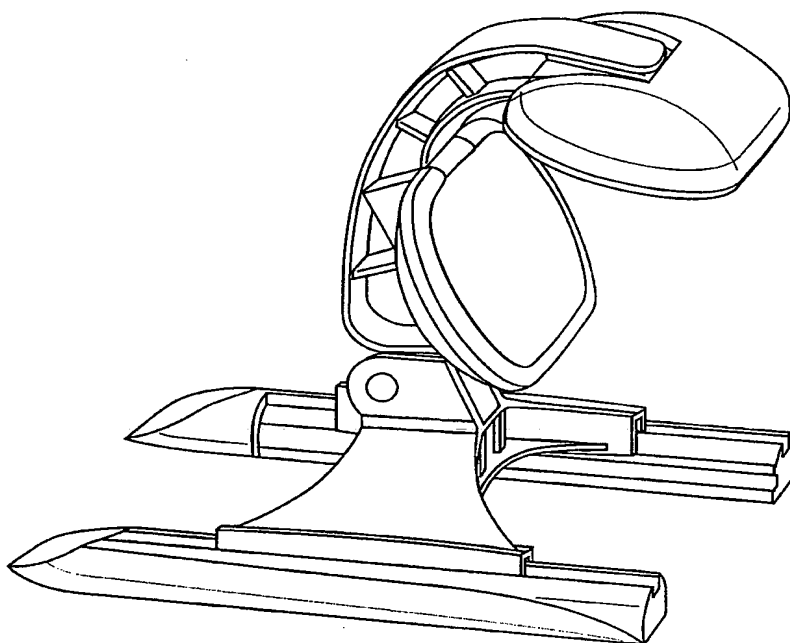


FIG. 21

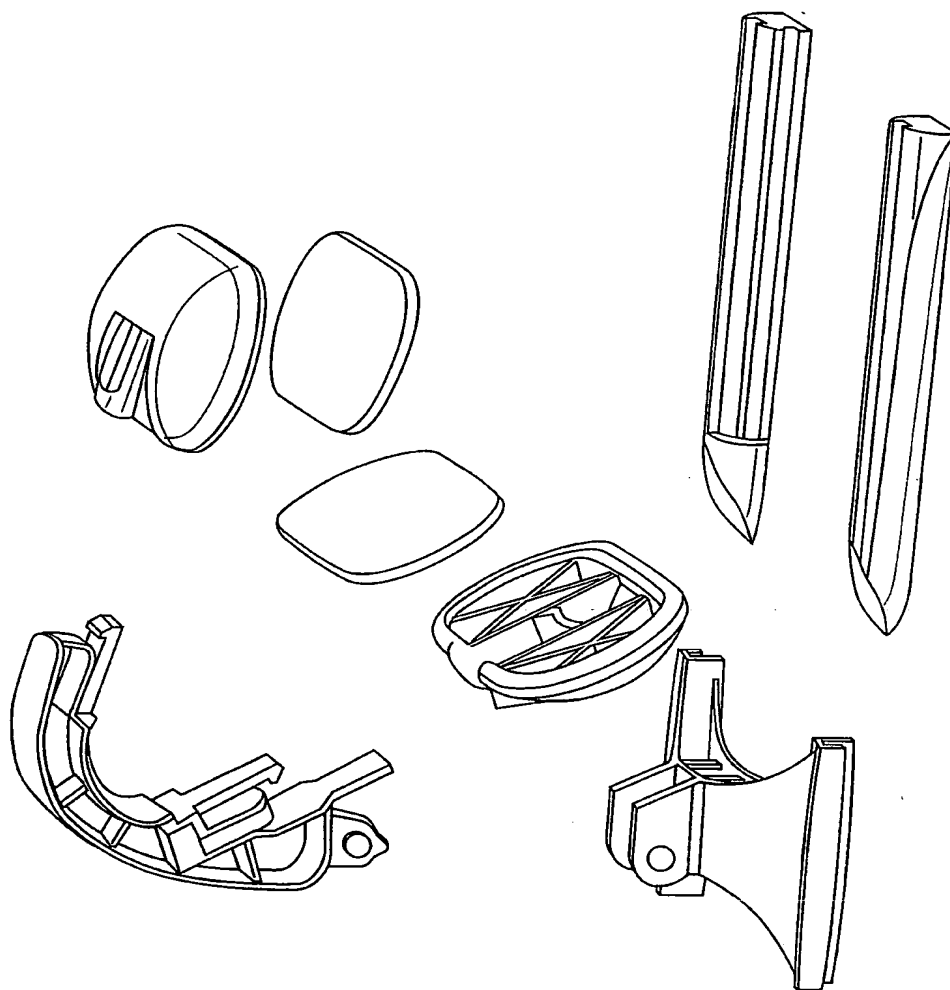


FIG. 22